

# Comparative Study of Blue Light with Ultraviolet (UVC) Radiations on SARS-CoV-2 Virus

Kritika vashishtha <sup>1</sup>, Fengfeng (Jeff) Xi <sup>2</sup>, and Alexandre Douplik <sup>2</sup>

<sup>1</sup>Ryerson University

<sup>2</sup>Affiliation not available

October 30, 2023

## Abstract

The ongoing coronavirus pandemic requires more effective disinfection methods. The disinfection using ultraviolet light (UV), especially longer UVCs such as 254 nm, 270/280 nm have been proved to have virucidal properties, but its adverse effects on human skin and eyes limit its use to enclosed unoccupied spaces. Several studies conducted in the past have shown the effectiveness of blue light (405nm) against bacteria and fungi, but the virucidal property of 405nm has largely been unexplored. Based on previous studies, visible light mediates inactivation by absorbing the porphyrins and reacting with oxygen to produce reactive oxygen species (ROS). This causes oxidative damage to biomolecules such as protein, lipids, and nucleic acids, essential constituents of any virus. The virucidal potential of visible light has been speculated because the virus lacks porphyrins. This study demonstrated porphyrin independent viral inactivation and a comparative analysis of the effectiveness of 405nm against other UVC wavelengths. The beta coronavirus 1 (strain OC43) was treated against 405nm, 270/280nm, 254nm, and 222nm, and its efficacy was determined using median tissue culture infectious dose, i.e., TCID<sub>50</sub>. The results support the disinfection potential of visible light technology by providing a quantitative effect that can serve as a basic groundwork for future visible light inactivation technologies. In the future, blue light technology usage can be widened to hospitals, public places, aircraft cabins, and/or infectious laboratories to inactivate SARS-CoV-2.

# Comparative Study of Blue Light with Ultraviolet (UVC) Radiations on SARS-CoV-2 Virus

Kritika Vashishtha<sup>1</sup>, Fengfeng Xi<sup>2</sup>, Priya Dharmalingam<sup>3</sup>, and Alexandre Douplik<sup>4</sup>

<sup>1,2</sup>Department of Aerospace Engineering, Ryerson University, Toronto, Canada

<sup>3</sup>Department of Mechanical Engineering, Ryerson University, Toronto, Canada

<sup>4</sup>Department of Physics, Ryerson University, Toronto, Canada

Corresponding author: Kritika Vashishtha (e-mail: kvashishtha@ryerson.ca).

**ABSTRACT** The ongoing coronavirus pandemic requires more effective disinfection methods. The disinfection using ultraviolet light (UV), especially longer UVCs such as 254 nm, 270/280 nm have been proved to have virucidal properties, but its adverse effects on human skin and eyes limit its use to enclosed unoccupied spaces. Several studies conducted in the past have shown the effectiveness of blue light (405nm) against bacteria and fungi, but the virucidal property of 405nm has largely been unexplored. Based on previous studies, visible light mediates inactivation by absorbing the porphyrins and reacting with oxygen to produce reactive oxygen species (ROS). This causes oxidative damage to biomolecules such as protein, lipids, and nucleic acids, essential constituents of any virus. The virucidal potential of visible light has been speculated because the virus lacks porphyrins. This study demonstrated porphyrin independent viral inactivation and a comparative analysis of the effectiveness of 405nm against other UVC wavelengths. The beta coronavirus 1 (strain OC43) was treated against 405nm, 270/280nm, 254nm, and 222nm, and its efficacy was determined using median tissue culture infectious dose, i.e., TCID<sub>50</sub>. The results support the disinfection potential of visible light technology by providing a quantitative effect that can serve as a basic groundwork for future visible light inactivation technologies. In the future, blue light technology usage can be widened to hospitals, public places, aircraft cabins, and/or infectious laboratories to inactivate SARS-CoV-2.

**INDEX TERMS** Visible light, 405nm, Virucidal, Inactivation, SARS-CoV-2, Irradiation, Far-UVC, 222nm

## I. INTRODUCTION

The severe acute coronavirus 2 (SARS-CoV-2) pandemic has been an ongoing concern since its major outbreak in 2019, affecting the health and lives of millions of people across the world. While several unprecedented measures have been taken to control its spread such as vaccinating people against the virus and strict sanitization measures have been quite effective in combatting the ill effects of the virus. As of February 2022, more than 10 billion doses of vaccines have been administered across the globe [1]. Rigorous sanitization, which uses 60 to 95% ethyl alcohol, has well-established benefits and has thus been adopted by most households to clean surfaces and hands. However, despite strict sanitization, the virus is still spreading and affecting millions of people globally, which points out the need for more effective disinfection technologies.

Ultraviolet (UV) is an invisible part of the electromagnetic spectrum which ranges from 100 to 400 nm. The UV range is mainly categorized into three sections based on

wavelength. The range from 100 to 280nm comes under -UVC; the range from 280nm to 320nm as UVB; and 320 to 400nm as UVA [2]. The lower range of UVC wavelengths between 200 to 222 nm is termed as Far-UVC. UVC is absorbed by the ozone layer but due to its antimicrobial properties it has been artificially created and used for disinfection purposes for the past few centuries. The most used UVC wavelength has been 254nm and it has well-established efficacy against bacteria, fungi, and viruses. Other UVC wavelengths such as 260-280nm have also shown the potential to inactivate the virus.

## II. BACKGROUND

A study [3] conducted in past used 260nm, a combination of 260/280nm and 280nm to treat viruses. The required fluences (UV doses) were approximately 8 mJ/cm<sup>2</sup> for coxsackievirus A10 and poliovirus 1, 10 mJ/cm<sup>2</sup> for enterovirus 70, and 13 mJ/cm<sup>2</sup> for echovirus 30 [3]. Amongst these three, 260nm was more effective for enteroviruses and 280nm showed relatively higher efficacy for human

adenovirus (a DNA virus) [3]. Though UVCs have proven inactivation potential, they can cause severe burns on the skin, eye injuries like photokeratitis on human eyes, skin [4]. Additionally, the effect of UVC radiations on materials raises concerns about compromising the structural integrity or the premature aging of the products [5].

In the last decade, far-UVC has gained huge popularity for its higher irradiation power, resulting in low dose requirements for inactivation of bacteria, fungi, and viruses and also its lower penetration in human live tissue compared to 254nm, making it safer for human exposure [6]. Former studies on the antimicrobial property of far-UVC have demonstrated its capacity to inactivate the influenzas and coronaviruses in the air at a dose that does not damage the human cells [7] [8]. Prior research has a dearth of data on the long-term effects of far-UVC and its exposure to human eyes.

The way UVC light attacks pathogens are different for different wavelengths. The structure of SARS-CoV-2 contains structural proteins i.e., spikes(S), envelope(E), membrane(m), and nucleocapsid(N) proteins [9]. The SARS-CoV-2 uses its spikes protein to attach to the host cell. Once it's inside the host cell, it multiplies and kills the cells [10]. The two ways UVC attacks the virus are either by viral genome damage (DNA/RNA) or viral protein damage. For viral genome damage, the UVC range from 200 to 280nm is absorbed by the deoxyribonucleic acid (DNA) and ribonucleic acid (RNA) through the formation of pyrimidine dimers [11]. The 254nm causes genome damage which prevents the virus from replicating. However, the DNA can repair itself in the presence of blue light through the process called photo-reactivation [12]. The 222nm, however, can cause both genome damage and protein damage because 222nm is absorbed more by structural proteins in contrast to 254nm [13]. Among shorter wavelengths (200 to 230nm) range, 222nm has been more effective than 210nm and 230nm [13].

The visible blue light ranges from 400-470nm, and in the current study, we have used 405nm for the inactivation of the SARS-CoV-2 virus. Unlike UVC, visible light is considered safe for human skin and eyes [14]. Furthermore, a study [15] conducted showed the comparative analysis of the degradative effects of UVC and 405nm on endoscope tube material. The UVC caused substantial photodegradation damage whereas 405 had no notable detrimental effect [15]. Lower irradiation blue light dose had shown inactivation for bacteria like *Clostridium* spp and *Listeria* spp [16] [17], fungal species such as *Saccharomyces* spp and *Candida* spp [18], and a higher dose on viruses like feline calicivirus (FCV)30 [19], and viral hemorrhagic septicemia virus (VHSV) [20]. The mechanism of inactivation by blue light is by absorbing the light via photosensitizers such as porphyrins and reacting with oxygen or any other cell components [21] [22]. This produces a reactive oxygen species (ROS) which causes oxidative damage [21] [22]. The non-selective nature of ROS

can cause direct damage to biomolecules such as protein, lipids, and nucleic acids which are essential constituents of bacteria, fungi, and viruses [21] [22]. As the virus lacks porphyrins, the virucidal property of blue light is highly speculated. Most of the research conducted used porphyrins to inactivate the virus in the media. In this study, the media had no porphyrins, and the test was conducted without the use of external photosensitizers. A recent study also showed the inactivation of SARS-CoV-2 and influenza A H1N1 without the use of photosensitizer [23]. Nevertheless, mechanisms by which blue light causes nonselective damage to the virus is still unknown. A future investigation is required to understand the mechanism through which blue light causes inactivation.

The dose requirement varies with wavelengths and pathogens. The wavelengths below 240nm can more readily generate ozone [24] thus should be a deciding factor for dose determination. The dose of 222nm used was 3mJ/cm<sup>2</sup> for this study. Whereas for 254nm and 270/280nm, a slightly higher dose of 10mJ/cm<sup>2</sup> was used. For 405nm measured a higher dose of 17280mJ/cm<sup>2</sup> was used.

The goal of this study is to investigate blue light (405nm) inactivation efficacy against the virus and compare it with far-UVC (222nm), standard mercury bulbs(254nm), and LED UVC (270/280nm). In what follows, a comparative study for the blue light with the three UVC lights and described their efficacy of Covid-19 virus disinfection.

### III. METHODOLOGY

#### A. LIGHT SOURCES

The 405nm LED (Fig. 1) light manufacturer used in this study was DIEHL Aviation [25]. The LED prototype uses the same mechanical component as the regular mini spotlight. The light has the peak wavelength at 405nm with measured spectral power distribution. The LED light has a single mode with constant power wattage.


The 222nm light used was from manufacturer Ushio Care222, krypton-chloride (Kr-Cl) excimer lamp module. The typical excimer lamp emits peak irradiation at 222nm alongside a longer UVC wavelength whereas, Ushio uses a special short-pass filter to block other UVC wavelengths that are above 230nm [26] (Fig. 2).

The Ushio germicidal low-pressure mercury arc lamp emits peak radiation of 253.7nm (Fig. 3).

The 270/280nm was from manufacturer GMKJ. Each led module shown in Fig. 4A was connected in a three-corner arrangement. Each module has the same peak wavelength and same irradiance power. The specifications of UVC led used are shown in Table I. DC voltage from the main power supply is applied to each UV-led module in accordance with the available current.



The viral sample in the petri dish was exposed to the irradiance of  $1.80E-03 \text{ W/cm}^2$ ,  $9.18E-04 \text{ W/cm}^2$ ,  $3.50E-03 \text{ W/cm}^2$ , and  $3.47E-05 \text{ W/cm}^2$  from the light sources 405nm, 222nm, 254nm, and 270/280nm respectively.

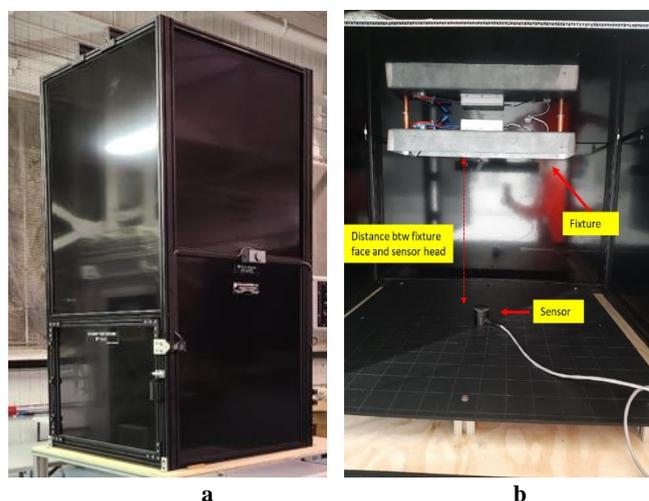

**Figure 2. a) Test Rig b) Inside test rig showing the fixture to install the light source and the sensor to measure the irradiance ( $\text{mW/cm}^2$ )**

### C. CELLS AND VIRUS PREPARATION

The HCT8 cells (CCL244) purchased from ATCC were cultured according to the manufacturer's protocol. The cells were grown in a complete medium prepared by supplementing RPMI 1640 medium with 10% horse serum (Gibco; 26050070) and 1% penicillin-streptomycin (Gibco; 15 140122). The cells culture flask was placed in the incubator maintained at  $37^\circ\text{C}$  with 5%  $\text{CO}_2$ . Beta coronavirus 1 strain OC43 (VR-1558) purchased from ATCC is propagated using host cell HCT8. All the experiments involving OC43 were conducted within the biosafety level 2 safety cabinet at the Toronto St. Michaels Hospital facility. Viral stocks were prepared by infecting the confluent monolayers of HCT8 cells with OC43. Initial viral absorption is allowed for 1-2 hours with continuous rocking, and then the cells were supplied with an infection medium consisting of RPMI1640 supplemented with 2% horse serum. The virus-infected cells were incubated at  $37^\circ\text{C}$  with 5%  $\text{CO}_2$  and monitored for 4-6 days or until achieving an 80% cytopathic effect. The produced viral stocks were stored at  $-80^\circ\text{C}$  for further use.


### D. TCID50

The commonly used Polymerase Chain Reaction (PCR) test does not apply to our test as it measures virus infection. Instead, TCID50 assay was used to measure the infectivity of the virus, i.e., virus inactivation. TCID50 represents a dilution of virus that makes 50% of the test wells showing cell detachment. The infectivity titer is expressed as TCID50/ml. To perform TCID50, host cells (HCT-8) ( $1.5 \times 10^4$  cells in  $100 \mu\text{l}$ ) in complete medium were plated in a 96-well plate (Cryo Vial Holder) (Fig. 6a). Incubate the plates for 16-24 h

at  $37^\circ\text{C}$  in a 5%  $\text{CO}_2$  incubator to achieve 80% confluency of the cells. To prepare the virus for infection, dilute  $100 \mu\text{l}$  of virus from stock to  $900 \mu\text{l}$  of serum-free media (10-1 dilution) and make subsequent 10-fold serial dilutions of the virus (10-2 to 10-10 dilution). On day 1, remove the culture medium from each well. Inoculate  $100 \mu\text{l}$  of the virus solution to each well. Aliquots of the same sample are inoculated in multiples of 4 wells. Incubate the plates for 1 h at  $37^\circ\text{C}$  in a 5%  $\text{CO}_2$  incubator. After incubation, remove the inoculum and add an overlay infection medium containing 2% horse serum. Incubate the plates at  $37^\circ\text{C}$  in a 5%  $\text{CO}_2$  incubator and observe the cytopathic effect (CPE) for 6-12 days. Using an inverted microscope (Fig. 6 b), count the number of wells with or without CPE. TCID50/ml is then calculated using the Reed-Muench method [28].



**Figure 3. a) TCID50 (with virus samples)**

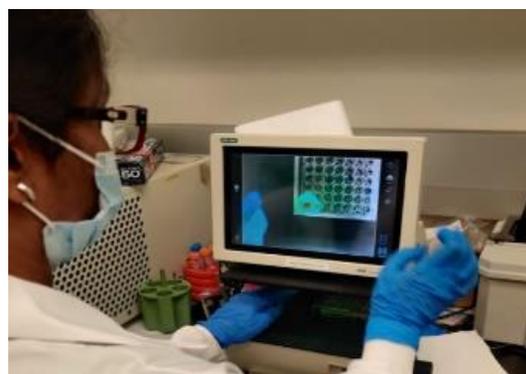

**Figure 6. b) Cryo Vial Holder with virus sample under a microscope**

## IV. RESULT

To visually investigate the efficiency of ultraviolet rays, a randomly chosen 270/280nm source was used to treat the virus sample with a dose of  $10\text{mJ/cm}^2$ , and basic infectivity results are shown in Fig. 7. Fig. 7a shows the control sample (no UV more conclusive and quantitative results, TCID50 was conducted.

The irradiance( $\text{mW/cm}^2$ ) for each light source was measured at 10cm distance which is shown in Table II below and based on measured irradiance and required dose, the exposure time was calculated using equation (1). The inactivation efficiency based on dose and exposure time was calculated using the TCID50. For 405nm the virus was exposed to  $1720\text{mJ/cm}^2$  for

2hours 40 minutes and a reduction of log10 2.84 was observed i.e., is 99.85%. For 222nm the virus sample was exposed to 3mJ/cm<sup>2</sup> for 3.27seconds which resulted in log10 2.50 reduction i.e., 99.68%. For 254nm and 270/280nm ultraviolet rays, the virus samples were exposed to 10mJ/cm<sup>2</sup> for 3.26 seconds and 288.18seconds respectively, which resulted in log10 3.17, i.e., is 99.93% and log10 3.37 i.e., is 99.95% reduction. After each test, the test rig was cleaned with ethyl alcohol, and the treated samples were stored in the dark at 4°C. 405nm required the highest dose and maximum exposure time to reach 2.84 log reduction. The summarized results are shown in Table III.

Table II

Shows irradiance(W/cm2) for different UVCs and blue light at different distances

Distance btw the virus sample and fixture(cm)	Irradiance(W/cm <sup>2</sup> )			
	405nm	222nm	254nm	270/280nm
10	1.80E-03	9.18E-04	3.50E-03	3.47E-05
20	4.46E-04	3.17E-04	1.03E-03	7.33E-06
30	1.98E-04	1.32E-04	5.29E-04	2.83E-06
40	1.15E-04	8.09E-05	3.19E-04	1.43E-06
50	7.36E-05	5.08E-05	2.12E-04	8.51E-07

Table III

Showing TCID50 result for treated virus sample, the dose used, and exposure time for different UVCs and blue light

Light Source	Distance (cm)	Irradiance (W/cm <sup>2</sup> )	Exposure Time (s)	Dose (mJ/cm <sup>2</sup> )	TCID50	
					Log Reduction	%
405	10	1.80E-03	9600	17280	2.84	99.85%
222	10	9.18E-04	3.27	3	2.50	99.68%
254	10	3.50E-03	3.26	10	3.17	99.93%
270/280	10	3.47E-05	288.18	10	3.34	99.95%

## V. DISCUSSION

The ongoing pandemic is in dire need of uninterrupted inactivation technology. Visible blue light inactivation has indicated the log reduction of 2.84 (that is a 99.85% reduction), which is a significant reduction. The irradiation used in this study was 1.8mW/cm<sup>2</sup> and the exposure time was 2 hours and 40 minutes.

The mechanism by which visible blue light attacks the virus is still unknown and in past studies, external photosensitizers were used in the medium. In this research, 405nm (Fig. 8 shows the visible blue light in our setup) caused inactivation to virus without the presence of any external photosensitizers. Before using visible light for continuous inactivation, its photobiological hazards to humans should be studied. The IEC 62471 [14] standards have taken into consideration the skin, cornea, and retinal hazard. These hazards depend on wavelengths, physiological sensitivity to various wavelengths, angular subtense, and exposure time.

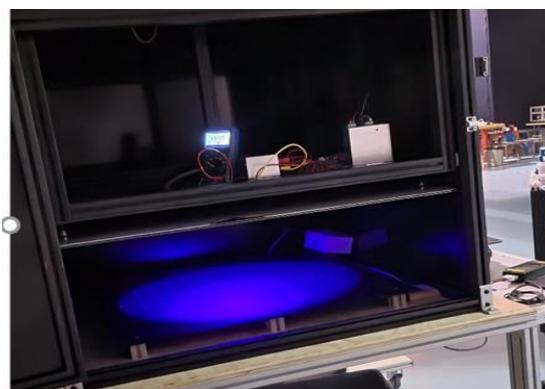


Figure 8. Demo of DIEHL 405nm Light

The brief mention of eyes anatomy is pertinent for understanding the angular subtense. The basic parts of the eyes are the retina, cornea, pupil, lens, and conjunctiva. The pupil is the small opening that allows the light into the eye and behind the pupil is the lens that focuses the light energy density on the retina. The superficial part of the eye is the cornea and conjunctiva. The amount of light that enters the eye depends on how big the pupil is. The pupil's average maximum constriction and dilation are about the diameter of 3mm and 7mm, respectively. This diameter is a limiting factor to correspond to the field of view (FOV). It is assumed that the pupil remains constricted to a diameter of 3mm for visible light, whereas, for wavelengths outside the visible range, the pupil is dilated. Exposure time also determines the field of view. For disinfection purposes, the exposure time is more than 10000seconds. The exposed area of the retina will be around a FOV angle of 0.1 radians which is over 5 degrees.

By IEC 62471 [14], the skin or cornea hazard by blue light is denoted by E<sub>B</sub>. The equation provided by the IEC standard for E<sub>B</sub> is for small sources, i.e., the aperture less than 0.011 [14]. The skin and cornea hazard (E<sub>B</sub>) ranges from low risk at 1.0 W.m<sup>-2</sup> and moderate risk at 400 W.m<sup>-2</sup>. LB denotes retinal hazard, and the value is based on radiance (W.m<sup>-2</sup>.sr<sup>-1</sup>). The LB limit ranges from low risk at 10000 W.m<sup>-2</sup>.sr<sup>-1</sup> and moderate risk at 4000000 W.m<sup>-2</sup>.sr<sup>-1</sup>.

The human exposed to a light source with radiance lower than 100 W.m<sup>-2</sup>.sr<sup>-1</sup> will receive a dose of greater than 10<sup>6</sup> J.m<sup>-2</sup>.sr<sup>-1</sup> in 10000seconds exposure time (2hours and 45 minutes), and this is classified as no risk [29]. If exposed to a light source of radiance higher than 100W.m<sup>-2</sup>.sr<sup>-1</sup> but less than W.m<sup>-2</sup>.sr<sup>-1</sup>, the person will receive the dose greater than 10<sup>6</sup> J.m<sup>-2</sup>.sr<sup>-1</sup> within 100seconds exposure time; and this is classified as low risk [29]. The light source whose radiance is higher than 10,000 W.m<sup>-2</sup>.sr<sup>-1</sup> is classified as medium to high risk, and that light source is prohibited from domestic general lighting [29]. There are many commercial lights like vital vio [30] that have been tested for IEC 62471 [14] and have been placed in Exempt Group (RG O) i.e. it poses no optical hazard for continuous, unrestricted exposure to humans. The skin and cornea hazard is determined in irradiance, whereas retinal hazard is considered radiance. Assuming that only domestic general visible blue light is used for disinfection which means

retinal hazard is already considered and only skin and cornea hazard must be calculated for uninterrupted disinfection purposes.

The inverse square law can be used to draw irradiance and the distance dependence assuming the constant angular position ( $\theta = 0^\circ$ ). From Fig. 9, the curve equation can be used to calculate the intermittent irradiance value at different distances for the same blue light source used in this study, which can be further used to calculate the dose ( $\text{mJ}/\text{cm}^2$ ).

#### Irradiance ( $\text{mW}/\text{cm}^2$ ) vs Distance (r)

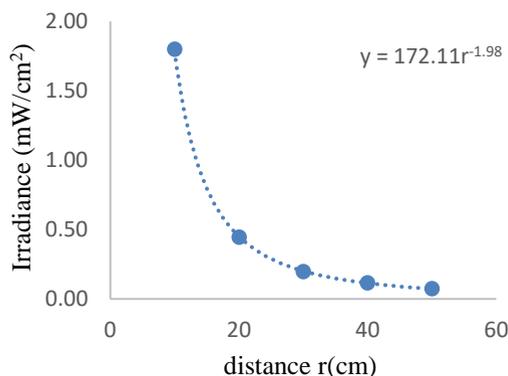


Figure 4. Illustration of inverse square law for calculating irradiance for DIEHL blue light source

## VI. CONCLUSION

The 405nm exposure resulted in a log reduction of 2.84 in 2 hours and 40 minutes. For safety reasons, the beta coronavirus was used and not the SARS-CoV-2, as there have been many reported accidental cases of usage of SARS-CoV-2 [31]. Based on the results and discussed advantages of using 405nm over UVC, the 405nm deployment in public arenas seems pragmatic and doable. Therefore, 405nm can potentially inactivate the coronavirus, and its limitation of slower inactivation rate in comparison to UVCs can be resolved by using multiple light sources with irradiance being within the acceptable range provided by IEC 62471 [14]. Ergo, blue light technology can be the first of its kind for uninterrupted disinfection.

## REFERENCES

- [1] T. Randall, S. Cedric, A. Tartar and P. Murray, "Vaccine Tracker," 01 Feb 2022. [Online]. Available: <https://www.bloomberg.com/graphics/covid-vaccine-tracker-global-distribution/>.
- [2] "What is ultraviolet radiation?," 11 07 2017. [Online]. Available: <https://www.canada.ca/en/health-canada/services/sun-safety/what-is-ultraviolet-radiation.html>.
- [3] H. Woo, E. S. Beck, A. L. Boczek, M. K. Carlson, E. N. Brinkman and G. K. Linden, "Efficacy of Inactivation of Human Enteroviruses by Dual-Wavelength Germicidal Ultraviolet (UV-C) Light Emitting Diodes (LEDs)," *water*, vol. 11, no. 6, p. 1131, 30 May 2019.
- [4] "Ultraviolet (UV) Radiation," 19 08 2020. [Online]. Available: <https://www.fda.gov/radiation-emitting-products/tanning/ultraviolet-uv-radiation>.
- [5] M. Matthew, "Testing the Effects of UV-C Radiation on Materials," *International Surface Technology*, vol. 14, no. 2, pp. 46-47, 29 July 2021.
- [6] J. Childress, J. Roberts and T. King, *Disinfection with Far-UV (222 nm Ultraviolet Light)*, 2020.
- [7] M. Buonanno, D. Welch and I. Shuryak, "Far-UVC light (222 nm) efficiently and safely inactivates airborne human coronaviruses," *Scientific Reports*, vol. 10, no. 1, 24 June 2020.
- [8] W. David, M. Buonanno, V. Grilj, I. Shuryak, C. Crickmore, A. W. Bigelow, G. Randers-Pehrson, G. W. Johnson and J. D. Brenner, "Far-UVC light: A new tool to control the spread of airborne-mediated microbial diseases," *Scientific Reports*, vol. 8, no. 1, p. 2752, 09 Feb 2018.
- [9] K. Fatimab, T. Mohammada, I. K. Singh, A. Singh, M. S. Atif, G. Hariprasad and M. G. Hasan, "Insights into SARS-CoV-2 genome, structure, evolution, pathogenesis and therapies: Structural genomics approach," *Biochim Biophys Acta Mol Basis Dis*, vol. 1866, no. 10, p. 165878, 01 10 2020.
- [10] G. Simmons, J. Reeves, A. Rennekamp, S. Amberg, A. Piefer and P. Bates, "Characterization of severe acute respiratory syndrome-associated coronavirus (SARS-CoV) spike glycoprotein-mediated viral entry," *Proceedings of the National Academy of Sciences of the United States of America*, vol. 101, no. 12, p. 4240-4245, 23 Mar 2004.
- [11] G. Pfeifer, Y. You and A. Besaratinia, "Mutations induced by ultraviolet light.," *Mutation Research*, vol. 571, no. 1-2, pp. 19-31, 01 Apr 2005.
- [12] K. O. Oguma, H. Katayama and S. Ohgaki, "Photoreactivation of Escherichia coli after Low- or Medium-Pressure UV Disinfection Determined by an Endonuclease Sensitive Site Assay," *Journal of Clinical Microbiology*, vol. 68, no. 12, pp. 6029-6035, 12 2002.
- [13] M. Hessling, R. Haag, N. Sieber and P. Vatter, "The impact of far-UVC radiation (200-230 nm) on pathogens, cells, skin, and eyes - a collection and analysis of a hundred years of data," *GMS hygiene and infection control*, vol. 16, p. Doc07, 16 Feb 2021.
- [14] "CLC EN 62471:2008 Photobiological safety of lamps and lamp systems," 11 Sept 2008. [Online]. Available: <https://standards.iteh.ai/catalog/standards/clc/a50af9ae-9590-4282-ba82-91f666fe52a7/en-62471-2008>.
- [15] D. Irving, A. D. Lamprou, M. Maclean and et al, "A comparison study of the degradative effects and safety implications of UVC and 405 nm germicidal light sources for endoscope storage," *Polymer Degradation and Stability*, vol. 133, pp. 249-254, November 2016.
- [16] L. J. Murrell, E. K. Hamilton and H. B. Johnson, "Influence of a visible-light continuous environmental disinfection system on microbial contamination and surgical site infections in an orthopedic operating room," *American Journal of Infection Control*, vol. 47, no. 7, pp. 804-810, 07 2019.
- [17] M. Maclean, L. E. Murdoch, S. J. MacGregor and J. G. Anderson, "Sporicidal effects of high-intensity 405 nm visible light on endospore-forming bacteria," *Photochemistry and Photobiology*, vol. 89, no. 1, pp. 120-126, 30 Jan 2013.
- [18] L. E. Murdoch, K. Mckenzie, M. Maclean, S. J. Macgregor and J. G. Anderson, "Lethal effects of high-intensity violet 405-nm light on *Saccharomyces cerevisiae*, *Candida albicans*, and on dormant and

germinating spores of *Aspergillus niger*," *Fungal Biology*, vol. 117, no. 7-8, pp. 519-527, 07 2013.

- [19] R. M. Tomb, M. Maclean and J. E. Coia, "New Proof-of-Concept in Viral Inactivation: Virucidal Efficacy of 405 nm Light Against Feline Calicivirus as a Model for Norovirus Decontamination," *Food and Environmental Virology*, vol. 9, no. 2, pp. 159-167, 06 2017.
- [20] D. T. Diem Tho Ho, K. Ahran and K. Nameun , "Effect of blue light emitting diode on viral hemorrhagic septicemia in olive flounder (*Paralichthys olivaceus*)," *Aquaculture*, vol. 521, p. 735019, 2020.
- [21] D. Tianhong , . G. Asheesh and M. K. Clinton , "Blue light for infectious diseases: *Propionibacterium acnes*, *Helicobacter pylori*, and beyond?," *Drug Resistance Updates*, vol. 15, no. 4, pp. 223-236, 28 July 2012.
- [22] V. .V. Bumah, E. Aboulizadeh and D. . S. Masson-Meyers, "Spectrally resolved infrared microscopy and chemometric tools to reveal the interaction between blue light (470nm) and methicillin-resistant *Staphylococcus aureus*," *Journal of Photochemistry and photobiology*, vol. 167, pp. 150-157, 23 Dec 2016.
- [23] R. Rathnasinghe, S. Jangra, L. Miorin, M. Schotsaert, C. Yahnke and A. Garcia-Sastre, "The Virucidal effects of 405 nm visible light on SARS-CoV-2 and influenza A virus," vol. 11, no. 1, p. 19470, 30 09 2021.
- [24] C. Holger, "Ozone Generation by Ultraviolet Lamps," *Photochemistry and Photobiology*, vol. 97, no. 3, pp. 471-476, 03 February 2021.
- [25] "DIEHL Aviation," Accessed Mar 25, 2022. [Online]. Available: <https://www.diehl.com/aviation/de/portfolio/cabin-lighting/>.
- [26] "Care222 Science," 2022. Accessed Mar 25, 2022. [Online]. Available: <https://care222.com/care222-science/>
- [27] "International Light Technologies," Accessed Mar 25, 2022. [Online]. Available: <https://www.intl-lighttech.com/products/ilt2400-xsd140a>.
- [28] M. . A. Ramakrishnan and M. Dhanavelu, "Influence of Reed-Muench Median Dose Calculation Method in Virology in the Millennium," *Antiviral Research*, vol. 28, no. 2, pp. 16-18, December 2018.
- [29] S. Point, "Blue Light Hazard: Are exposure limit values protective enough for newborn infants?," *EDP Sciences*, vol. 53, no. Radioprotection, pp. 219 - 224, 12 July 2018.
- [30] A. Fields, "The Impact of Vital Vio Antibacterial Light," 2019.
- [31] W. Lim, K.-C. Ng and D. N. C. Tsang, "Laboratory containment of SARS virus," *Annals of the Academy of Medicine, Singapore*, vol. 35, no. 5, pp. 354-360, 2006.




simulation, and visual comfort

**KRITIKA VASHISHTHA** received her bachelor's degree in manufacturing engineering from India in 2016. She is currently pursuing PhD from Ryerson University, Toronto, Canada, in Aerospace Engineering. Her research interest includes photonics, circadian rhythm, light



**FENGFENG XI** is professor with the Department of Aerospace Engineering at Ryerson University. He received his PhD degree from University of Toronto. He was the Director of Ryerson Institute for Aerospace Design and Innovation (RIADI) for the last ten years. Currently, he holds a Senior Industrial Research Chair position supported by the Natural Sciences and Engineering Research Council of Canada (NSERC). The focus of his current research is placed on the development of intelligent systems for the enhancement of air travel comfort including lighting, acoustics, and seating. Dr. Xi has served as the Conference Chair for the 2021 IEEE International Conference on Reconfigurable Mechanisms and Robots (ReMAR) and is an associate editor for Robotics and Computer-Integrated Manufacturing (RCIM) and a guest editor for Robotica



**PRIYA DHARMALINGAM** is a postdoctoral fellow in the Department of mechanical and industrial engineering at Ryerson University. She recently received her Ph.D. degree from Ryerson University. She was a recipient of the Ontario Trillium scholarship. Her current research interests are functionalizing nanoparticles for cancer diagnosis, gene delivery, and cancer therapy. She was also working closely with industrial partners for developing technologies to test antiviral coatings for aircraft cabins.



**ALEXANDRE DOUPLIK** is a Professor and Head of Ryerson Photonics Group in Physics Department at Ryerson University since 2011, and a Scientist of St. Michael's Hospital, Toronto, specializing in Advanced Optical Biomedical Imaging and Laser Surgery and Therapy. He is the author of more than 60 peer-reviewed papers, 70 conference papers, 6 book chapters, and 15 patents. In 2008-2011 he was a contract (non-tenure-track) Research Professor/Habilitation of Nuremberg-Erlangen University, Germany where he defended his Biomedical Engineering Habilitation (Dr. of Science degree) in 2011. Before 2007 he was Scientific Associate at Biophysics/Bioimaging Division in Ontario Cancer Institute in Toronto (2006-2007) and Senior Researcher of Xillix Technologies Corp., Vancouver (2002-2006).

